

Contents

1. Description
 - 1.1 Principle
 - 1.2 Background information
 - 1.3 Applications
 - 1.4 Reagent and instrument requirements
2. Protocol
 - 2.1 Reagent preparation
 - 2.2 Sample preparation
 - 2.2 Staining of SARS-CoV-2 RBD-specific B cells
3. Example of immunofluorescent staining using the SARS-CoV-2 RBD B Cell Analysis Kit, anti-human

Warnings

Reagents contain sodium azide. Under acidic conditions sodium azide yields hydrazoic acid, which is extremely toxic. Azide compounds should be diluted with running water before discarding. These precautions are recommended to avoid deposits in plumbing where explosive conditions may develop.

1. Description

This product is for research use only.

Components	10 µg Recombinant SARS-CoV-2 RBD (HEK)-Biotin – research grade 60 µL Streptavidin, PE 60 µL Streptavidin, PE-Vio® 770 60 µL CD19 Antibody, anti-human, APC-Vio 770 (clone: LT19, isotype: mouse IgG1κ) 60 µL CD27 Antibody, anti-human, Vio Bright FITC (clone: M-T271, isotype: mouse IgG1κ) 60 µL IgG Antibody, anti-human, VioBlue® (clone: IS11-3B2.2.3, isotype: mouse IgG1κ) 60 µL IgA Antibody, anti-human, VioGreen™ (clone: IS11-8E10, isotype: mouse IgG1κ) 60 µL IgM Antibody, anti-human, APC (clone: PJ2-22H3, isotype: mouse IgG1) 1 mL 7-AAD Staining Solution
Capacity	30 tests for up to 2×10^8 total B cells or 4×10^8 peripheral blood mononuclear cells (PBMCs).
Product format	Antibodies are supplied in buffer containing stabilizer and 0.05% sodium azide. The ready-to-use 7-AAD Staining Solution is supplied in phosphate-buffered saline, pH 7.2, at a concentration of 52.5 µg/mL. Recombinant SARS-CoV-2 RBD (HEK)-Biotin – research

grade, human is supplied lyophilized from a filtered (0.2 µm) buffer solution.

Storage

Store fluorochrome-conjugated antibodies and 7-AAD Staining Solution protected from light at 2–8 °C. Do not freeze. Store Recombinant SARS-CoV-2 RBD (HEK)-Biotin at –20 °C. Upon reconstitution aliquots should be stored at –20 °C or below. Avoid repeated freeze-thaw cycles. The expiration dates are indicated on the vial labels.

1.1 Principle

The SARS-CoV-2 RBD B Cell Analysis Kit, human has been developed for the fast and easy detection of SARS-CoV-2-specific B cells by binding of the SARS-CoV-2-specific proteins to the respective antigen-specific B cell receptor (BCR) on B cells circulating in the peripheral blood of individuals who developed a B cell response against SARS-CoV-2 proteins. The kit contains SARS-CoV-2 recombinant proteins and Streptavidin conjugates to prepare RBD-tetramer solutions (tetramers formed from Recombinant SARS-CoV-2 RBD (HEK)-Biotin with Streptavidin, PE and PE-Vio 770, respectively). Fluorochrome-conjugated antibodies in the kit allow the identification and phenotyping of the B cells (memory B cells and isotypes), and the 7-AAD Staining Solution is used for the exclusion of dead and apoptotic cells. The optimized antibody panel and protocol ensure an easy and efficient analysis of SARS-CoV-2-specific B cells.

1.2 Background information

The quantitative and qualitative analysis of antigen-specific B cells specifically recognizing and reacting towards a defined antigen provides important information to understand their function in various immunological situations. The presence of these cells indicate that an individual is mounting an adaptive response to the specific, infective pathogen or to an immunization containing that specific antigen. Infection with severe acute respiratory syndrome coronavirus 2 (SARS-CoV-2) induces an adaptive immune response leading to SARS-CoV-2-specific immunoglobulins and SARS-CoV-2-specific memory B and memory T cells with variable persistency and antiviral efficacy. Analysis and enrichment of antigen-specific B cells can contribute to the understanding of the role of cellular and humoral responses and thus to the protection from SARS-CoV-2 infection after a previous infection or immunization.

1.3 Applications

Identification and characterization of SARS-CoV-2-specific B cells circulating in peripheral blood of individuals who developed a B cell response against SARS-CoV-2 proteins:

- Sensitive and specific quantification of the numbers of antigen specific B cells.
- Phenotyping of the differentiation status and isotype (IgG, IgA, IgM) of SARS-CoV-2-specific B cells.
- Cell sorting of SARS-CoV-2-specific B cells.

1.4 Reagent and instrument requirements

- Phosphate-buffered saline (PBS), pH 7.2, without azide, protein, or other amine-containing compounds.
- PEB buffer: Prepare a solution containing phosphate-buffered saline (PBS), pH 7.2, 0.5% bovine serum albumin (BSA), and 2 mM EDTA by diluting MACS® BSA Stock Solution (# 130-091-376) 1:20 with autoMACS® Rinsing Solution (# 130-091-222). Keep buffer cold (2–8 °C).
- Flow cytometer equipped with a red (640 nm), a blue (488 nm), and a violet (405 nm) laser, e.g., MACSQuant® Analyzer 10 (# 130-096-343) or MACSQuant Analyzer 16 (# 130-109-803).
- (Optional) REAlease® CD19 MicroBead Kit, human (# 130-117-034) for pre-enrichment of B cells.
- (Optional) StemMACS™ Cryo-Brew (# 130-109-558) for cryopreservation of B cells after pre-enrichment.
- (Optional) 8-Color Immunophenotyping Kit, anti-human, REAfinity (# 130-120-640) for quality control of the PBMC samples.
- (Optional) MACS Comp Bead Kit, anti-human Igk (# 130-104-187) for optimal compensation of the fluorescence spillover from fluorochrome-conjugated antibodies.

2. Protocol

2.1 Reagent preparation

▲ Volumes given below are for up to 5×10^6 B cells or 10^7 PBMCs. When working with fewer cells, use the same volumes as indicated. When working with higher cell numbers, scale up all reagent volumes and total volumes accordingly (e.g. for 10^7 B cells, use twice the volume of all indicated reagent volumes and total volumes).

1. Resuspend Recombinant SARS-CoV-2 RBD (HEK)-Biotin in deionized, sterile-filtered water to a final concentration of 0.1 mg/mL (e.g. use 100 μ L water for 10 μ g protein).

▲ **Note:** To avoid repeated freeze-thaw cycles prepare working aliquots from the stock solution of Recombinant SARS-CoV-2 RBD (HEK)-Biotin. Store the working aliquots at -70 °C. Once thawed the protein can be stored for up to three days at 2–8 °C.

2. Prepare both RBD-tetramer solutions by mixing Recombinant SARS-CoV-2 RBD (HEK)-Biotin, PEB buffer, and Streptavidin, PE or PE-Vio 770 (50 μ g/mL), respectively, as indicated in table 1. Incubate for 15 minutes at room temperature.

▲ **Note:** Always freshly prepare the RBD-tetramer solutions before use. Do not store the solutions.

RBD-tetramer solution	Recombinant SARS-CoV-2 RBD (HEK)-Biotin	Streptavidin fluorochrome	PEB buffer
RBD-tetramer-PE	0.75 μ L	0.6 μ L Streptavidin, PE	3.65 μ L
RBD-tetramer-PE-Vio 770	1.5 μ L	1.2 μ L Streptavidin, PE-Vio 770	7.3 μ L

Table 1: Volumes for preparation of RBD-tetramer solutions for one test with 5×10^6 B cells. Note that handling of small volumes below 1 μ L might cause imprecisions. Therefore, it is recommended to scale up reagents to prepare solution with bigger volumes.

3. Prepare the antibody staining cocktail: For each test mix 2 μ L of each fluorochrome-conjugated antibody, 5 μ L of 7-AAD Staining Solution, 5 μ L of RBD-tetramer-PE, and 10 μ L of RBD-tetramer-PE-Vio 770. Fill up to 100 μ L with PEB buffer.

2.2 Sample preparation

When working with anticoagulated peripheral blood or buffy coat, peripheral blood mononuclear cells (PBMCs) should be isolated by density gradient centrifugation, for example, using Ficoll-Paque™.

▲ **Note:** To remove platelets after density gradient separation, resuspend cell pellet in buffer and centrifuge at 200 \times g for 10–15 minutes at 20 °C. Carefully aspirate supernatant. Repeat washing step.

For details refer to the protocols section at www.miltenyibiotec.com/protocols.

2.3 Staining of SARS-CoV-2 RBD-specific B cells


▲ CD19⁺ cells can be enriched from single-cell suspension of PBMCs using the REAlease CD19 MicroBead Kit. Follow the instructions in the data sheet.

1. Resuspend 5×10^6 B cells or 10^7 PBMCs in 100 μ L of antibody staining cocktail. Incubate for 30 minutes at 2–8 °C.
2. Wash cells by adding 1–2 mL of PEB buffer and centrifuge at 300 \times g for 10 minutes. Aspirate supernatant completely.
3. Resuspend cell pellet in suitable amount of PEB buffer and analyze by flow cytometry using a suited flow cytometer, e.g. the MACSQuant Analyzer 16.

3. Example of immunofluorescent staining using the SARS-CoV-2 RBD B Cell Analysis Kit, anti-human

PBMCs of COVID-19 convalescent and healthy donors were obtained by density centrifugation. B cells were enriched using the REAlease CD19 MicroBead Kit, human. Cells were used fresh or cryopreserved in StemMACS Cryo-Brew.

Samples of label-free B cells were stained using the SARS-CoV-2 RBD B Cell Analysis Kit, human and analyzed by flow cytometry using the MACSQuant Analyzer 10. Cell debris, doublets, and dead cells were excluded from the analysis based on scatter signals and 7-AAD fluorescence. Afterwards, CD19⁺ cells were gated and RBD-specific B cells were detected using the double discrimination method.

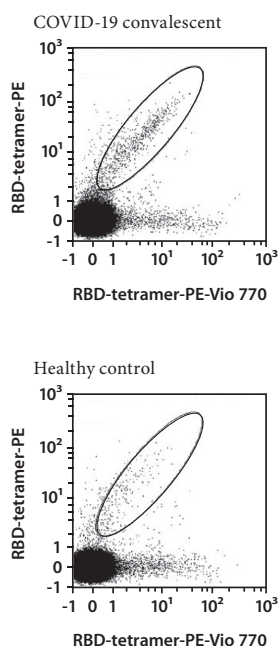

Refer to www.miltenyibiotec.com for all data sheets and protocols. Miltenyi Biotec provides technical support worldwide. Visit www.miltenyibiotec.com for local Miltenyi Biotec Technical Support contact information.

Legal notices

Limited product warranty

Miltenyi Biotec B.V. & Co. KG and/or its affiliate(s) warrant this product to be free from material defects in workmanship and materials and to conform substantially with Miltenyi Biotec's published specifications for the product at the time of order, under normal use and conditions in accordance with its applicable documentation, for a period beginning on the date of delivery of the product by Miltenyi Biotec or its authorized distributor and ending on the expiration date of the product's applicable shelf life stated on the product label, packaging or documentation (as applicable) or, in the absence thereof, ONE (1) YEAR from date of delivery ("Product Warranty"). Miltenyi Biotec's Product Warranty is provided subject to the warranty terms as set forth in Miltenyi Biotec's General Terms and Conditions for the Sale of Products and Services available on Miltenyi Biotec's website at www.miltenyibiotec.com, as in effect at the time of order ("Product Warranty"). Additional terms may apply. BY USE OF THIS PRODUCT, THE CUSTOMER AGREES TO BE BOUND BY THESE TERMS.

THE CUSTOMER IS SOLELY RESPONSIBLE FOR DETERMINING IF A PRODUCT IS SUITABLE FOR CUSTOMER'S PARTICULAR PURPOSE AND APPLICATION METHODS.

Technical information

The technical information, data, protocols, and other statements provided by Miltenyi Biotec in this document are based on information, tests, or experience which Miltenyi Biotec believes to be reliable, but the accuracy or completeness of such information is not guaranteed. Such technical information and data are intended for persons with knowledge and technical skills sufficient to assess and apply their own informed judgment to the information. Miltenyi Biotec shall not be liable for any technical or editorial errors or omissions contained herein.

All information and specifications are subject to change without prior notice. Please contact Miltenyi Biotec Technical Support or visit www.miltenyibiotec.com for the most up-to-date information on Miltenyi Biotec products.

Licenses

This product and/or its use may be covered by one or more pending or issued patents and/or may have certain limitations. Certain uses may be excluded by separate terms and conditions. Please contact your local Miltenyi Biotec representative or visit Miltenyi Biotec's website at www.miltenyibiotec.com for more information.

The purchase of this product conveys to the customer the non-transferable right to use the purchased amount of the product in research conducted by the customer (whether the customer is an academic or for-profit entity). This product may not be further sold. Additional terms and conditions (including the terms of a Limited Use Label License) may apply.

CUSTOMER'S USE OF THIS PRODUCT MAY REQUIRE ADDITIONAL LICENSES DEPENDING ON THE SPECIFIC APPLICATION. THE CUSTOMER IS SOLELY RESPONSIBLE FOR DETERMINING FOR ITSELF WHETHER IT HAS ALL APPROPRIATE LICENSES IN PLACE. Miltenyi Biotec provides no warranty that customer's use of this product does not and will not infringe intellectual property rights owned by a third party. BY USE OF THIS PRODUCT, THE CUSTOMER AGREES TO BE BOUND BY THESE TERMS.

Trademarks

autoMACS, MACS, MACSQuant, the Miltenyi Biotec logo, StemMACS, REAlease, Vio, VioBlue, and VioGreen are registered trademarks or trademarks of Miltenyi Biotec and/or its affiliates in various countries worldwide.

Ficoll-Paque is a trademark of GE Healthcare companies

Copyright © 2022 Miltenyi Biotec and/or its affiliates. All rights reserved.