

## Contents

1. Description
  - 1.1 Principle of the MACS® Separation
  - 1.2 Background information
  - 1.3 Applications
  - 1.4 Reagent and instrument requirements
2. Protocol
  - 2.1 Preparation of Leukopak®
  - 2.2 Magnetic labeling
  - 2.3 Magnetic separation
3. Example of a separation using the StraightFrom Leukopak® CD3 MicroBeads, human

## 1. Description

This product is for research use only.

<b>Components</b>	2×4 mL StraightFrom Leukopak® CD3 MicroBeads, human
	MicroBeads conjugated to monoclonal anti-human CD3 antibodies (isotype: mouse IgG2a).
<b>Capacity</b>	For one ½ Leukopak®.
<b>Product format</b>	StraightFrom Leukopak® CD3 MicroBeads, human are supplied in buffer containing stabilizer and 0.05% sodium azide.
<b>Storage</b>	Store StraightFrom Leukopak® CD3 MicroBeads, human protected from light at +2 to +8 °C. Do not freeze. The expiration date is indicated on the vial or box label.

### 1.1 Principle of the MACS® Separation

First, the CD3<sup>+</sup> cells in a Leukopak® sample are magnetically labeled with StraightFrom Leukopak® CD3 MicroBeads, human. Then, the cell suspension is loaded onto a Multi-24 Column Block, which is placed in the magnetic field of a MACS® Separator. The magnetically labeled CD3<sup>+</sup> cells are retained within the column. The unlabeled cells run through; this cell fraction is thus depleted of CD3<sup>+</sup> cells. After removing the column from the magnetic field, the magnetically retained CD3<sup>+</sup> cells can be eluted as the positively selected cell fraction.

### 1.2 Background information

During leukapheresis white blood cells are separated from whole blood and collected as highly concentrated leukocytes in Leukopaks®, which are ideal for the isolation of large numbers of various leukocyte subsets.

StraightFrom Leukopak® CD3 MicroBeads, human have been

developed for the positive selection of CD3<sup>+</sup> cells directly from one Leukopak® by using the MultiMACS™ Cell24 Separator Plus. No sample preparation is required, including density gradient centrifugation or erythrocyte lysis. The CD3 antigen is associated with the T cell receptor (TCR) heterodimer. CD3 is expressed on all T cells, constituting 15–20% of human peripheral blood leukocytes.

### 1.3 Applications

- Isolation of CD3<sup>+</sup> cells from Leukopak®. The purified CD3<sup>+</sup> cells are well suited for further flow cytometric, functional, or molecular analysis.

### 1.4 Reagent and instrument requirements

- Separation buffer: Prepare a solution containing phosphate-buffered saline (PBS), pH 7.2, 0.5% bovine serum albumin (BSA), and 2 mM EDTA by diluting MACS BSA Stock Solution (# 130-091-376) 1:20 with autoMACS® Rinsing Solution (# 130-091-222). Keep buffer cold (+2 to +8 °C). Alternatively, use autoMACS Running Buffer. Degas buffer before use, as air bubbles could block the column.  
 ▲ **Note:** BSA can be replaced by other proteins such as human serum albumin, human serum, or fetal bovine serum (FBS). Buffers or media containing Ca<sup>2+</sup> or Mg<sup>2+</sup> are not recommended for use.
- 1× Whole Blood Column Elution Buffer (# 130-131-889).
- 2× Multi-24 Column Block (# 130-095-692).
- MultiMACS Cell24 Separator Plus (# 130-098-637).
- 24-well Deep Well Plates (# 130-110-500) or Single-well Deep Well Plates (# 130-114-966).
- (Optional) Fluorochrome-conjugated antibodies for flow cytometric analysis, e.g., CD3 Antibody, anti-human. For more information about antibodies refer to [www.miltenyibiotec.com/antibodies](http://www.miltenyibiotec.com/antibodies).
- (Optional) Propidium Iodide Solution (# 130-093-233) or 7-AAD Staining Solution (# 130-111-568) for flow cytometric exclusion of dead cells.

## 2. Protocol

▲ StraightFrom Leukopak® CD3 MicroBeads, human have been developed for positive selection of target cells from one ½ Leukopak® with up to 200 mL (5×10<sup>9</sup>–1×10<sup>10</sup> cells). When working with smaller volumes, scale down all reagents and total volumes accordingly (e.g. for ¼ Leukopak®, fill up to 100 mL and use 4 mL StraightFrom Leukopak® CD3 MicroBeads, human and one Multi-24 Column Block). When working with higher volumes per ½ Leukopak®, contact Technical Support.

## 2.1 Preparation of Leukopak®

1. Divide a ½ Leukopak® equally into two collection tubes (max. 100 mL per tube). If the volume per tube is less than 100 mL, fill up to 100 mL with separation buffer.
2. Proceed to magnetic labeling (2.2).



## 2.2 Magnetic labeling

▲ Work fast, keep cells cold, and use pre-cooled solutions. This will prevent capping of antibodies on the cell surface and non-specific cell labeling.

▲ Volumes for magnetic labeling given below are for one tube containing 100 mL sample. Repeat labeling and separation steps for each tube one after the other.

▲ The recommended incubation temperature is +2 to +8 °C. Higher temperatures and/or longer incubation times may lead to non-specific cell labeling. Working on ice may require increased incubation times.

1. Add 4 mL StraightFrom Leukopak® CD3 MicroBeads, human the tube containing 100 mL sample.
2. Mix well by inverting the tube and incubate for 15 minutes in the refrigerator (+2 to +8 °C).
3. Proceed directly to magnetic separation (2.3).



## 2.3 Magnetic separation

▲ For more detailed instructions on how to use the MultiMACS Cell24 Separator Plus, refer to the user manual.

▲ The MultiMACS Cell24 Separator Plus, including the MACS Elution Station, has to be used with two Multi-24 Column Block and four Deep Well Plates for magnetic separation with StraightFrom Leukopak® MicroBeads.

▲ **Note:** For equilibration of the second column block use the Deep Well Plate from the first column block equilibration. Use one Deep Well Plate for collection of the positive fractions from both column blocks. To reach maximum cell recovery, rinse the Deep Well Plate after removal of the positive fraction and combine with the positive fraction. For collection of the negative fraction and the wash fractions, use two Deep Well Plates.

▲ Buffer volumes per column are as follows:

Equilibration: 2 mL separation buffer

Wash: 3×1 mL separation buffer

Elution: 1 mL Whole Blood Column Elution Buffer


▲ Divide the sample equally between the 24 columns of the Multi-24 Column Block, e.g., when the starting volume is 104 mL (100 mL Leukopak® and 4 mL StraightFrom Leukopak® MicroBeads), add 4.33 mL onto each column. Proceed with separation. Repeat steps for the second tube.

▲ Select the program **POSSEL2** and follow the on-screen instructions of the MultiMACS Cell24 Separator Plus.

▲ After separation, centrifuge the positive fraction at 200×g for 10 minutes. Aspirate supernatant carefully. Resuspend cell pellet in a suitable amount of buffer or medium for subsequent analysis.

## 3. Example of a separation using StraightFrom Leukopak® CD3 MicroBeads, human

Separation of a Leukopak® sample using StraightFrom Leukopak® CD3 MicroBeads, human and the MultiMACS Cell24 Separator Plus with the Multi-24 Column Blocks. Cells were fluorescently stained with CD3-FITC, CD14-VioGreen™, and CD45-VioBlue® and analyzed by flow cytometry using the MACSQuant® Analyzer. Cell debris and dead cells were excluded from the analysis based on scatter signals, propidium iodide fluorescence, and CD45 expression.

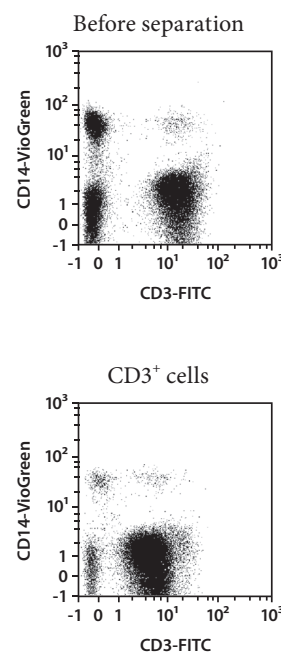

Refer to [www.miltenyibiotec.com](http://www.miltenyibiotec.com) for all data sheets and protocols. Miltenyi Biotec provides technical support worldwide. Visit [www.miltenyibiotec.com](http://www.miltenyibiotec.com) for local Miltenyi Biotec Technical Support contact information.

## Legal notices

### Limited product warranty

Miltenyi Biotec B.V. & Co. KG and/or its affiliate(s) warrant this product to be free from material defects in workmanship and materials and to conform substantially with Miltenyi Biotec's published specifications for the product at the time of order, under normal use and conditions in accordance with its applicable documentation, for a period beginning on the date of delivery of the product by Miltenyi Biotec or its authorized distributor and ending on the expiration date of the product's applicable shelf life stated on the product label, packaging or documentation (as applicable) or, in the absence thereof, ONE (1) YEAR from date of delivery ("Product Warranty"). Miltenyi Biotec's Product Warranty is provided subject to the warranty terms as set forth in Miltenyi Biotec's General Terms and Conditions for the Sale of Products and Services available on Miltenyi Biotec's website at [www.miltenyibiotec.com](http://www.miltenyibiotec.com), as in effect at the time of order ("Product Warranty"). Additional terms may apply. BY USE OF THIS PRODUCT, THE CUSTOMER AGREES TO BE BOUND BY THESE TERMS.

THE CUSTOMER IS SOLELY RESPONSIBLE FOR DETERMINING IF A PRODUCT IS SUITABLE FOR CUSTOMER'S PARTICULAR PURPOSE AND APPLICATION METHODS.

### Technical information

The technical information, data, protocols, and other statements provided by Miltenyi Biotec in this document are based on information, tests, or experience which Miltenyi Biotec believes to be reliable, but the accuracy or completeness of such

information is not guaranteed. Such technical information and data are intended for persons with knowledge and technical skills sufficient to assess and apply their own informed judgment to the information. Miltenyi Biotec shall not be liable for any technical or editorial errors or omissions contained herein.

All information and specifications are subject to change without prior notice. Please contact Miltenyi Biotec Technical Support or visit [www.miltenyibiotec.com](http://www.miltenyibiotec.com) for the most up-to-date information on Miltenyi Biotec products.

## Licenses

This product and/or its use may be covered by one or more pending or issued patents and/or may have certain limitations. Certain uses may be excluded by separate terms and conditions. Please contact your local Miltenyi Biotec representative or visit Miltenyi Biotec's website at [www.miltenyibiotec.com](http://www.miltenyibiotec.com) for more information.

The purchase of this product conveys to the customer the non-transferable right to use the purchased amount of the product in research conducted by the customer (whether the customer is an academic or for-profit entity). This product may not be further sold. Additional terms and conditions (including the terms of a Limited Use Label License) may apply.

CUSTOMER'S USE OF THIS PRODUCT MAY REQUIRE ADDITIONAL LICENSES DEPENDING ON THE SPECIFIC APPLICATION. THE CUSTOMER IS SOLELY RESPONSIBLE FOR DETERMINING FOR ITSELF WHETHER IT HAS ALL APPROPRIATE LICENSES IN PLACE. Miltenyi Biotec provides no warranty that customer's use of this product does not and will not infringe intellectual property rights owned by a third party. BY USE OF THIS PRODUCT, THE CUSTOMER AGREES TO BE BOUND BY THESE TERMS.

## Trademarks

autoMACS, MACS, MACSQuant, the Miltenyi Biotec logo, MultiMACS, StraightFrom, VioBlue, and VioGreen are registered trademarks or trademarks of Miltenyi Biotec B.V. & Co. KG and/or its affiliates in various countries worldwide. All other trademarks mentioned in this publication are the property of their respective owners and are used for identification purposes only.

Leukopak is a registered trademark of StemExpress LLC.

Copyright © 2024 Miltenyi Biotec and/or its affiliates. All rights reserved.